



Europäisches Patentamt  
European Patent Office  
Office européen des brevets

Publication number:

0 078 636  
A1

B36

## EUROPEAN PATENT APPLICATION

Application number: 82305597.5

Int. Cl.: G 01 N 27/30, G 01 N 33/48

Date of filing: 21.10.82

Priority: 23.10.81 GB 8132034

Applicant: Genetics International, Inc., 50 Milk Street  
Fifteenth Floor, Boston, MA 02109 (US)  
Applicant: Higgins, Irving John, Lion Fields Barford  
Road, Wilton Bedfordshire (GB)

Date of publication of application: 11.05.83  
Bulletin 83/19


Inventor: Higgins, Irving John, Lion Fields Barford Road,  
Wilton Bedfordshire (GB)  
Inventor: Hill, Hugh Allen Oliver, 9 Clover Close, Oxford  
(GB)  
Inventor: Plotkin, Elliot Verne, 14 George Street, Bedford  
Bedfordshire (GB)

Designated Contracting States: BE CH DE FR GB IT LI  
NL SE

Representative: Clifford, Frederick Alan et al, MARKS &  
CLERK 57/60 Lincoln's Inn Fields, London WC2A 3LS  
(GB)

Sensor for components of a liquid mixture.

A sensor electrode to detect one or more components in a liquid mixture comprises an electrically conductive material having at least at an external surface, the combination of an enzyme catalytic for a reaction of the desired component, and a mediator compound which transfers electrons from the enzyme to the electrode when such catalytic activity takes place. It can be used as an in vivo glucose sensor either with a silver electrode coated with e.g. glucose oxidase and a polyviologen as the mediator, or with a particulate carbon electrode, glucose oxidase and chloranil or fluoranil as mediator. Another system is to use bacterial glucose dehydrogenase or glucose oxidase as the enzyme and/or ferrocene or a ferrocene derivative as the mediator compound to give electrodes with improved linearity, speed of response and insensitivity to oxygen.



EP 0 078 636 A1

This invention relates to equipment and methods for detecting the presence of, measuring the amount of, and/or monitoring the level of one or more selected components in a liquid mixture.

5           While use may be made of this invention in chemical industry, especially where complex mixtures are encountered (e.g. in food chemistry or biochemical engineering) it is of particular value in biological investigation and control techniques. More particularly,  
10 it lends itself to animal or human medicine, and in particular to in vivo measuring or monitoring of components in body fluids.

For convenience, the invention will be described with reference primarily to one such procedure, the  
15 determination of glucose in a diabetic human subject, by the use of equipment which, while usable on a specific or occasional basis also lends itself to temporary or permanent implantation. However, while the provision of an implantable glucose sensor is a major object of  
20 the invention other and broader objects are not hereby excluded.

In vivo glucose sensors have already been proposed. One proposal is based on direct oxidation of

glucose at a catalytic platinum electrode (see Hormone and Metabolic Research, Supplement Series No. 8, pp 10-12 (1979))but suffers from the drawback of being non-specific and of being easily poisoned by interfering  
5 substances. Another proposal, for a procedure more specific to glucose, involves the use of glucose oxidase on an oxygen electrode (Adv. Exp.Med.Biol, 50 pp 189-197 (1974))but is not very responsive to the high glucose concentrations. Other systems using glucose oxidase  
10 have been proposed but not fully investigated for in vivo methods, see e.g. J..Solid-Phase Biochem. 4 pp 253 - 262 (1979).

The inventors have recently carried out in vitro studies of enzyme-catalysed reactions using a  
15 mediator in solution to transfer the electrons arising from the enzyme, during its action, directly to the electrode, as described in Biotechnology Letters 3 pp 187 - 192 (1981).

It has now been realised that mediator compounds  
20 can be associated with the sensor electrode structure thus rendering such electrodes available for use by in vivo methods.

In one aspect the present invention consists  
in a sensor electrode for use in liquid mixtures of  
25 components for detecting the presence of, measuring the

amount of, and/or monitoring the level of, one or more selected components capable of undergoing an enzyme-catalysed reaction, the electrode being composed of electrically conductive material and comprising, at least at an external surface thereof, the combination of an enzyme and a mediator compound which transfers electrons to the electrode when the enzyme is catalytically active.

Preferably the electrode is designed to determine glucose in vivo. The enzyme is therefore preferably a glucose oxidase, or possibly a glucose dehydrogenase, for example a bacterial glucose dehydrogenase.


Glucose oxidase ( $\beta$ -D-glucose:oxygen oxidoreductase, of enzyme classification EC 1.1.3.4) is a well known type of enzyme. Bacterial glucose dehydrogenase is of more recent discovery, and is believed to be a quinoprotein with a polycyclicquinone prosthetic group (PQQ). Reference is made to Duine et al TIBS, (Oct. 1981) 278 - 280 and Arch. Microbiol (1982) 131.27-31.

Use of such a bacterial glucose dehydrogenase in the present invention has certain advantages over the use of a glucose oxidase. The major advantage is that it can give an oxygen-insensitive glucose sensor, since the enzyme does not use oxygen as an electron acceptor. A suitable enzyme can be purified (as described in more

detail below) either by conventional chromatographic techniques or by two-phase aqueous partition from a range of micro-organisms. A preferred micro-organism is Acinetobacter calcoaceticus but various Gluconobacter species (e.g. Gluconobacter oxidans) or Pseudomonas species (e.g. Pseudomonas fluorescens, Pseudomonas aeruginosa) can also be used.

Mediator compounds which may be used in accordance with the invention are of different chemical types but all possess the electron-transfer property referred to above.

1. The mediator may for example be a polyviologen, for example, the type of material described in J. Polym. Sci. 13 pp 1 - 16 (1975), J. Appln. Polym. Sci. 24 pp 2075 - 85 (1979) or J. Polym. Sci. 17 pp 3149-57 (1979). A specific preferred polyviologen is that compound made from o-dibromo xylene and 4,4'-bipyridyl, according to the following reaction:-

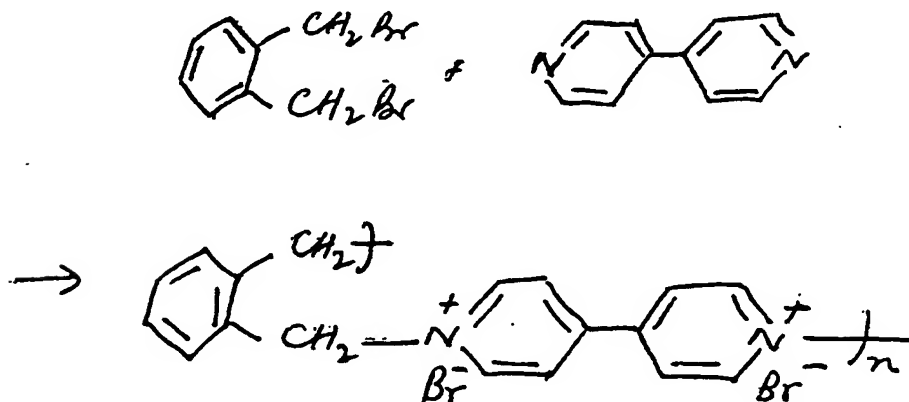

and described in Polymer Letters 9 pp 289-295 (1971).

Such polyviologen material, as described below, can be coated over or bonded to electrodes.

It may include in its molecule long chain alkyl groups to increase its molecular weight and thus decrease its mobility.

2. The mediator may be a low-molecular weight compound of the group comprising chloranil, fluoranil or bromanil. The ortho-substituted isomers, and especially o-chloranil, are preferred within this class.

10 3. A particularly preferred form of mediator compound is a ferrocene or ferrocene derivative.

A ferrocene has, as its fundamental structure, an iron atom held "sandwiched" by dative bonds between two pentadienyl rings. It is an electroactive organometallic compound, acting as a pH-independent reversible one-electron donor. Various derivatives are available (e.g. with various substituents on the ring structure, possibly in polymer form) differing in redox potential, aqueous solubility and bonding constant to glucose oxidase or bacterial glucose dehydrogenase enzyme.

20 For instance, the redox potential of the parent compound is +422 mV vs NHE. By introducing functional groups on to the ring system,  $E^{\circ}$  can be varied between +300 and +650 mV. Moreover, the water-solubility of the carboxyl-substituted ferrocenes is greater than that of

the parent compound. Further description will be found in Kuwana T., 1977, ACS Symposium Series, 38, 154.

Among specific mediator compounds of this type are ferrocene itself, 1,1'-ferrocene dicarboxylic acid, dimethyl ferrocene, and polyvinyl ferrocene, e.g. of average molecular weight of about 16000.

4. Among further classes of mediator compounds for use in the present invention there figure
- 10 (a) compounds of biological origin and hence general compatibility with any proposed in vivo use, e.g. Vitamin K
  - (b) alkylsubstituted phenazine derivatives.

The electrically conductive material of the electrode itself can be a metal, particularly silver, or carbon either as a pre-formed rod or as an electrode shape made up from a paste of carbon particles. Surface condition of the electrode is usually important. If metal, the surface can be roughened where it contacts the active materials (enzyme and/or mediator). If solid carbon, the surface can be "oxidised" i.e. previously heat-treated in an oven with oxygen access.

Of the two types of enzyme listed, the dehydrogenase is preferred, and of the mediators the ferrocene-type compounds are preferred.

Certain combinations of the above materials, and certain configurations of electrode, are preferable in practice.

Polyviologens may be used with metallic electrodes. In one modification the invention envisages a metal electrode (preferably silver and with a roughened surface) coated with a mixture of glucose oxidase and a polyviologen described above, for example, in an agar layer and having a dialysis membrane located over this coating in order to prevent loss of active material while still allowing passage of the small glucose molecules.

Another modification of the invention provides a metal electrode coated with a stable film of glucose oxidase and a polyviologen co-immobilised on the metal surface e.g. by albumen and glutaraldehyde.

Yet another modification of the invention envisages a conductive electrode made of or including material to which a polyviologen is covalently bonded and further combined with glucose oxidase. The large polyviologen molecule projects from the electrode surface and this is believed to facilitate interaction with the enzyme.

In that form of the invention using poly-



8.

viologens, as exemplified in the three modifications above, it is an objective to keep loss of active material (enzyme or mediator) to a very low level i.e. by the surrounding membrane, co-immobilisation or covalent bonding. In a different form of the invention, however, still using glucose oxidase, a rather higher level of loss of active material is tolerated, giving a sensor electrode of reduced but still useful life, coupled with improved sensitivity and selectivity.

10 In this form of the invention the electrode is composed of particulate carbon mixed with a low molecular weight mediator disseminated throughout the electrode and glucose oxidase. Chloranil and/or fluoranil are useful mediator substances. It is envisaged  
15 to construct from such an electrode a replaceable sensor tip to a needle-type probe for projecting only into the dermis so as to allow ready replacement.

Optionally, enzyme immobilisation materials, or polymeric electrode admixtures e.g. TEFLON, or  
20 long-chain alkyl derivatives of mediators of increased molecular weight and thus decreased mobility, can be incorporated.

In a particularly valuable form of the invention, however, the electrode comprises a carbon core, a layer  
25 of ferrocene or a ferrocene derivative at a surface

thereof and a layer of glucose oxidase or glucose dehydrogenase at the surface of the ferrocene layer. The enzyme layer is preferably immobilised at the surface of the underlying mediator, retained in a self-sustaining gel layer thereupon and/or has a retention layer thereover permeable to the glucose molecule.

The carbon core can itself be solid or a stiff paste of particles. Normally, it will present a smooth surface for the ferrocene or ferrocene derivative, which may be adhered thereto in a number of ways, for example,

- (a) For a monomeric ferrocene or ferrocene derivative, by deposition from a solution in a readily evaporatable liquid e.g. an organic solvent such as toluene.
- (b) For a ferrocene polymeric derivative, deposition from a readily evaporable organic solvent for the polymer such as chloroform. J. Polymer Sci. 1976, 14 2433 describes preparation of a polyvinyl ferrocene of average molecular weight about 16000 which can be deposited in this way.
- (c) For a polymerisable ferrocene-type monomer, by electrochemically induced polymerisation in situ, e.g. by dissolving vinyl ferrocene in an organic electrolyte containing tertiary butyl ammonium perchlorate in concentration about 1M and depositing at a potential of - 700 mV

vinyl ferrocene radicals as a polymer in situ.

- (d) By covalent modification of the carbon electrode e.g. by carbo-diimide cross-linking of the ferrocene or ferrocene derivative on to the carbon.

5

The enzyme to be coated on to the ferrocene or ferrocene derivative can be the glucose oxidase or the bacterial glucose dehydrogenase. The glucose oxidase can be immobilised to the underlying surface e.g. by the carbo-diimide material DCC (1-cyclohexyl-3-(2-morpholino ethyl) carbo-diimide metho-p-toluene sulphonate) which gives a thin strongly bound layer, a good linear response to low glucose concentrations, and oxygen insensitivity (because of the competition from the ferrocene with oxygen for electrons transferred to the enzyme redox centre from the substrate). Using DCC immobilisation of glucose oxidase on ferrocene also extends the top end of the linear range of the sensor from about 2mM to 40mM.

10

15

20

Other methods of immobilisation, or other forms of protection e.g. incorporated into a self-supporting gelatine layer, are also possible.

The bacterial glucose dehydrogenase can also be immobilised at the mediator surface, but may be merely deposited from an evaporatable solution, or held in a gelatin layer.

25

Optionally, but preferably when being used on live blood, a protective membrane surrounds both the enzyme and the mediator layers, permeable to water and glucose molecules. This can be a film of dialysis membrane, resiliently held e.g. by an elastic O-ring. It can however also with advantage be a layer of cellulose acetate, e.g. as formed by dipping the electrode into a cellulose acetate solution in acetone.

It will be apparent that while the invention has primary relevance to a sensor electrode, especially such an electrode specific for glucose, it also relates to the combination of such an electrode and temporary or permanent implantation means, e.g. a needle-like probe. Also, such an electrode, connected or connectable, with signal or control equipment, more especially with an insulin administration means, constitutes an aspect of the invention. Moreover, a method of monitoring a diabetic subject involving the use of a temporarily or permanently implanted electrode as described above is also within the scope of the invention.

The electrodes according to the invention permit the manufacture of an improved macro-sensor for use in hospital analytical glucose-sensing instruments of the existing type. The advantages compared

to known instruments would be that the increased  
linear range together with very low oxygen sensitivity  
would allow omission of the dilution step involved  
in blood analysis in current instruments. Moreover,  
5 as described in more detail below, the response  
times of such electrodes are short (24 - 36 seconds  
for 95% of steady state depending on complexity of  
solution).

10 The electrodes of the invention, on the  
macro-scale could be incorporated into simple, cheap  
electronic digital read-out instruments for doctors  
surgeries or diabetic home-testing kits.

Use of a small version of the macro-sensor  
would be possible in a device which automatically  
15 takes a blood sample from the finger, brings it into  
contact with the sensor, amplifies the signal and  
gives a digital readout. Use of a micro-version of  
the sensor in a watch type device for monitoring glucose  
interstitial fluid in the skin could also be envisaged.  
20 It would be worn on the wrist and would have a dis-  
posable sensor cartridge in the back with one or more  
separate, fine, needle-type sensors. Each would feed  
into the electronics which if several sensors were  
used would cross-refer the current inputs to ensure  
25 reliability.

Connection of such devices to external insulin delivery systems could act as a feedback control loop for an insulin pump. Indeed, such a device could be housed in the canula used to feed insulin into the body from a pump and again serve as a sensor for the feedback loop. Other uses such as a hypoglycaemia alarm, or digital read-out monitor, are also possible.

The invention will be further described with reference to the following Examples 1 to 3 and to the accompanying drawings, in which:

Figure 1 is a diagrammatic longitudinal cross-section through a glucose sensor electrode,

Figure 2 is a diagrammatic longitudinal cross-section through a different form of glucose sensor electrode,

Figure 3 is a graph of the current sensed by the electrode of Figure 2, against glucose concentration,

Figure 4 is a diagrammatic longitudinal cross-section of the electrode of Figure 2 located within a hypodermic needle,

Figure 5 is a diagrammatic longitudinal cross-section through a yet further glucose sensor electrode,

Figure 6 is a graph analogous to Figure 3 for the electrode of Figure 5,

Figure 7 is a graph analogous to Figure 3 for an electrode incorporating a glucose dehydrogenase.

Example 1

Purification of Quinoprotein Glucose Dehydrogenase  
(GDH) from Acinetobacter calcoaceticus

(a) Growth of Organisms

Strain NCTC 7844 was grown on sodium succinate  
5 (20  $\text{gl}^{-1}$ ) in batch culture at pH 8.5 and 20°C. Cells  
were harvested after 20 hours ( $A_{600} = 6.0$ ) using a  
Sharples centrifuge, and stored frozen.

(b) Purification of Glucose Dehydrogenase

The method is based on the method of J A Duine  
10 et al (Arch Microbiol, 1982 vide supra) but with  
modifications as follows.

1. 100 g. of cells were thawed, resuspended in 3  
300 ml. of 56 mM Tris/39 mM glycine and treated for  
20 minutes at room temperature with 60 mg. lysozyme.
- 15 2. Triton X-100 extracts were combined and  
treated with 0.01  $\text{mgml}^{-1}$  of deoxyribonuclease I for  
15 minutes at room temperature. The resulting suspension  
was then centrifuged at 48000 xg for 25 minutes at 4°C.  
The supernatant from this centrifugation was then  
20 treated with ammonium sulphate. The yellow protein  
precipitating between 55 and 70% ammonium sulphate was  
resuspended in 36 mM Tris/39 mM glycine containing 1%  
Triton X - 100 and dialysed against that buffer at 4°C  
for 5 hours.
- 25 3. Active fractions from the CM sepharose C1-6B

15.

column were combined and concentrated using Millipore CX-30 immersible ultrafilters.

Example 2

Purification of Quinoprotein Glucose Dehydrogenase  
5 from Acinetobacter calcoaceticus (alternative method)

(a) Growth of Organisms

The method of Example 1 was repeated.

(b) Purification of GDH

The method is based on the partitioning of  
10 proteins between two liquid phases. The steps were:-  
1. Cells were thawed and resuspended at 3 ml/g  
wet weight in 50 mM sodium phosphate, pH 7.0. They were  
then pre-cooled on ice and passed once through a  
Stansted pressure cell (made by Stansted Fluid Power  
15 Ltd., Stansted, Essex, UK) at 25000 psi. This provided  
the cell-free extract.

2. The cell-free extract was then mixed for 15  
minutes at room temperature with 50% (w/v) polyethylene-  
20 glycol 1000, 50% (w/v) sodium phosphate, pH 7.0 and  
distilled water in the proportions of 2:4:3:1  
respectively. This mixture was centrifuged at 5000 rpm  
for 5 minutes to break the emulsion.

3. The lower layer was aspirated off and desalted  
25 immediately, by either diafiltration using an Amicon  
hollow-fibre ultrafiltration cartridge of 10000 mwt  
cut off, or by passage through a Sephadex G50 (medium  
grade) gel filtration column.



4. The resulting solution was concentrated using an Amicon PM10 membrane in a nitrogen pressure cell.

Example 3

5 Interaction between ferrocene and glucose oxidase

DC cyclic voltammetry was used to investigate the homogeneous kinetics of the reaction between ferrocene and the glucose oxidase enzyme under substrate  
10 excess conditions. A two compartment electromechanical cell of 1.0 ml volume fitted with a Luggin capillary was used. The cell contained a 4.0 mm gold disc working electrode, a platinum gauze counter-electrode and a saturated calomel electrode as a reference. A series  
15 of voltamograms for ferrocene was recorded at scan rates of  $1-1000 \text{ mVs}^{-1}$  in 50 mM potassium phosphate buffer, pH 7.0. The data showed that the mediator acted as a reversible, one-electron acceptor  $E_0^1 = +165 \text{ MV SCE}$ .

20 Addition of 50 mM glucose has no discernable effect on the electrochemistry of the mediator ( $500 \mu\text{M}$ ). Upon addition of glucose oxidase ( $10 \mu\text{M}$ ), however, an enhanced anodic current was observed in the voltamogram at oxidising potentials with respect to the mediator. This  
25 indicated catalytic regeneration of the reduced form of the mediator by glucose oxidase. Quantitative kinetic data was obtained for this reaction using an established

procedure (Nicholson, R.S. and Shain, J., 1964, Anal. Chem., 36, 707). The mediator gave a second order rate constant for the reaction between ferricinium ion and reduced glucose oxidase of  $K=10^4 \text{ m}^{-1} \text{ s}^{-1}$ . This  
5 ability of the ferricinium ion to act as a rapid oxidant for glucose oxidase facilitates the efficient coupling of the enzymic oxidation of glucose.

#### Example 4

The procedure of Example 3 was repeated using  
10 1,1'-ferrocene dicarboxylic acid instead of ferrocene. The value of  $E_o'$  was determined to be +420 mV, and the second order rate constant of the ferricinium ion and reduced glucose oxidase was again  $10^4 \text{ m}^{-1} \text{ s}^{-1}$ , thus confirming the conclusions drawn from Example 3.

#### 15 Example 5

##### Glucose oxidase/polyviologen

For experimental purposes an in vitro sensor was made up as shown in Figure 1.

A silver disc 1 was glued at 2 over the lower  
20 end of a length of 12 mm glass tubing 3. A wire 5 was soldered to the back of the silver disc at 6. The tubing was placed inside a "Teflon" sleeve 7, and the outside of the disc 1 roughened at 8. A solution containing glucose oxidase and the o-dibromo xylene/  
25 4, 4'-bipyridyl polyviologen was applied over the roughened

18.

surface 8 and dried to layer 9. A subsequent layer 10 of molten agar also containing the glucose oxidase and polyviologen, of approximately 1 mm in thickness was placed over the layer 9, and solidified. Finally, 5 dialysis membrane 11 was placed over the assembly and held by O-ring 12.

To demonstrate the principle of using the polyviologen mediator to couple electrically the glucose oxidase to an electrode, the sensor was placed 10 in a buffered electromechanical cell, which was stirred and agitated with a current of nitrogen. The electrode was held at -90mV vs SCE, and current flow measured on a chart recorder. Aliquots of glucose were added. As the glucose concentration in the solution 15 increased, over the range of 1 to 8mM, the current also increased, indicating that the electrode was acting as a glucose sensor.

#### Example 6

##### Glucose oxidase/Chloranil

20 Chloranil (10mg) was mixed with carbon powder (1.5g) and NUJOL (1ml) to form a paste and used as an electrode in a similar liquid system to the above. The electrical coupling between the enzyme and electrode was so effective that the enzyme preferentially reduced 25 the electrode rather than the oxygen, so that the system was oxygen-insensitive. The current response was linear

over the 1-10mM glucose concentration range.

19.

0078636

Example 7

Glucose/Oxidase Dimethyl Ferrocene

Mini electrode for in vivo glucose sensing in

5 skin

A graphite rod 13 (Figure 2) with an oxidised surface, 30 mm long x 0.9 mm diameter is glued with epoxy resin into a nylon tube 14 25 mm long, 0.9 mm inside diameter, 1.3 mm outside diameter. The end 15 of the electrode is dipped into a solution of dimethyl ferrocene, (10 mg/ml) in toluene, and the solvent is then allowed to evaporate.

The end 15 of the electrode is placed into a solution of water soluble DCC (25 mg/ml) in acetate buffer, pH 4.5 for 1 hour. It is then rinsed, in buffer only, for 5 minutes and thereafter placed in a solution of glucose oxidase (10 mg/ml) in acetate buffer, pH 5.5, for 1½ hours before again rinsing in buffer. The tip of the electrode 15, with the layers of dimethyl ferrocene and immobilised enzyme is then dipped into a solution of cellulose acetate dissolved in acetone and formamide and put into ice water for several minutes, to give a protected and stable electrode.

This electrode was connected to a potentiostat , together with a suitable counter electrode and calomel reference electrode and placed in a solution containing

glucose. The potential of the working electrode is kept at +100 mV to 300 mV relative to the calomel electrode, i.e. as low as possible to avoid oxidation of potentially interfering substances. A current is produced which is proportional to the glucose concentration. The time for 95% of response is less than 1 minute and the electrode gives a near linear response over the range 0 -32 mM glucose, as shown in Figure 3. Slow loss of activity ferrocene(due to slow loss of ferrocinium ion) can be minimised by keeping the electrode at a potential between 0 and -100mV vs. a standard calomel electrode when not in use.

Figure 4 shows in section an electrode structure in which an electrode (references as in Figure 2) of much smaller size is held within a hypodermic needle 16 plugged at its point 17 but with side windows 18 for passage of blood or other body fluid. The small size of such an electrode and its linear response over a large range of glucose concentrations makes it possible to use the electrode for in vivo glucose determination on both severely diabetic and normal individuals.

#### Example 8

##### Glucose Oxidase/Ferrocene

##### In vitro sensor

A carbon rod 19 (Figure 5) Ultra carbon, grade U5, 6 mm x 15 mm) with a metal connector 20 secured in one end was sealed in glass tubing 21 (borosilicate, 6 mm i.d. x mm) with an epoxy resin (araldite). (not shown). The exposed surface at 22 was polished with

emery paper and washed with distilled water. The entire rod was heated in an oven for 40 h at 200°C to given an oxidised surface at 22.

15  $15 \mu\text{l}$  of ferrocene (20 mg/ml in toluene) was pipetted onto the oxidised surface and allowed to dry completely. The rod was then placed in 1 ml of water-soluble DCC (25 mg/ml in 0.1M acetate buffer, pH 4.5) for 80 min at room temperature. The rod was then washed in 0.2 M carbonate buffer, pH 9.5 and placed in a glucose  
10 oxidase solution (Sigma type X, 12.5 mg/ml) for  $1\frac{1}{2}$  hours at room temperature. It was finally washed with water with a pH 7 buffer containing 0.2 g/l glucose) and stored at 4°C.

The characteristics of the above electrode  
15 were determined in a nitrogen-saturated buffer solution (0.2M  $\text{NaPO}_4$ , pH 7.3) and are shown in Figure 6. The curve is linear from 2 to 25 mM glucose and reaches saturation current at 100mM in glucose.

In separate tests with an air-saturated buffer  
20 at 8mM glucose the current was measured as being at least 95% of that produced in the nitrogen-saturated buffer.

Response time was also measured, being the time taken to achieve 95% of maximum current for the given glucose conc. With the nitrogen-saturated

buffer an electrode as described above had a response time of 24 seconds at 2mM glucose and 60 seconds at 6mM glucose. With the same buffer, such an electrode modified by a cellulose acetate membrane coating (produced  
5 as in Example 7) gave response times of 36 seconds (2mM) and 72 seconds (6mM). With blood, this modified electrode gave response times of 36 seconds (blood with a known 2mM glucose content) and 72 seconds (blood at a known 6mM glucose content).

10           Electrodes as above were stored in 20mM  $\text{NaPO}_4$ , pH7 for 4 weeks at 4°C as a stability test and thereafter re-examined as above. The results were within 10% and usually within 5% of results with a freshly made electrode.

#### Example 9

#### 15           Glucose Dehydrogenase/Ferrocene

A stiff carbon paste was made up from 1.6 g of Durco activated charcoal and 2.5 ml of liquid paraffin. A Pasteur pipette of 6 mm internal diameter was blocked 2mm from its wide end by a silver disc to which a  
20 connecting wire was soldered. The space between the disc and the end of the pipette was filled with the carbon paste, and the surface of the paste was polished with paper until smooth and even.

A single 20 microlitre drop of a toluene  
25 solution of ferrocene (20 mg/l) was placed on the

smooth surface and allow to spread and evaporate to leave a film of the ferrocene.

A further drop of 25 microlitres of bacterial glucose dehydrogenase solution as obtained in Example 1, containing between 1 and 10 mg. of protein per ml, was placed on this ferrocene surface and allowed to spread.

A cover of dialysis membrane was secured over the so-coated end of the electrode by a tight-fitting O-ring.

#### Example 10

##### Glucose Dehydrogenase/Ferrocene

The procedure of Example 9 was repeated but using as electrode the same carbon paste packed into the space defined between the end of a length of nylon tubing and a stainless steel hypodermic needle shaft inserted therein terminating 2 mm. short of the tubing end, so as to define a small electrode body. The electrode was further fabricated using only 5 microlitres of the ferrocene solution and 1 microlitre of the enzyme solution.

#### Example 11

##### Glucose Dehydrogenase/Ferrocene

The procedure of Example 9 was repeated using



as electrode a solid carbon rod (Ultracarbon grade U5 6 mm diameter) within a Pyrex glass tube 3 cm long and 6 mm internal diameter and connected to a stainless steel hypodermic shaft, giving a construction similar to that shown in Figure 5. The end of the carbon rod was polished smooth with emery cloth and aluminium oxide powder prior to the application of the ferrocene solution.

#### Example 12

##### 10      Glucose Dehydrogenase/Ferrocene

A gelation-entrapped glucose dehydrogenase was prepared by mixing at 37°C, 25 mg gelatin, 0.5 ml of the glucose dehydrogenase solution as described in Example 9 and 2.5 microlitres of TEMED.

15      After complete dissolving of the gelatin 200 microlitres of the solution was spread over an area of 2 cm<sup>2</sup> and allowed to dry under a stream of cold air.

A disc of 0.25 cm<sup>2</sup> area was then used instead of the drop of enzyme solution in Example 9.

##### 20      Example 13

##### Glucose Dehydrogenase/Ferrocene

Example 12 was repeated using a disc of the gel of 1 mm<sup>2</sup> area and applying it instead of the drops of enzyme solution in the construction of example 10.

The results obtained from the electrodes described in Examples 9 to 13 are all similar, and show a very specific electrode of low oxygen sensitivity. By way of example, the electrode of Example 12 was calibrated and gave the results shown in Figure 7.

Devices such as shown in the Examples offer advantages over most of the enzyme-based sensors currently available. When compared to such sensors prior to dilution steps, the present electrode has an equal or faster response time, the ability to operate under anaerobic conditions, greater oxygen insensitivity (important in blood samples, where oxygen concentration is variable), extended linear range covering the complete physiological range and comparable specificity, stability and ease of manufacture.

## CLAIMS:

1. A sensor electrode for use in a liquid mixture of components for detecting the present of, measuring the amount of, and/or monitoring the level of, one or more selected components capable of undergoing an enzyme-catalysed reaction, the electrode being composed of electrically conductive material, characterised in that it comprises at least at an external surface thereof, the combination of an enzyme and a mediator compound which transfers electrons to the electrode when the enzyme is catalytically active.
2. A sensor electrode as claimed in claim 1 characterised in that the enzyme catalyses a reaction of glucose whereby there is provided a glucose sensor.
3. A sensor electrode as claimed in claim 2 characterised in that the enzyme is a glucose oxidase.
4. A sensor electrode as claimed in claim 2 characterised in that the enzyme is a bacterial glucose dehydrogenase.
5. A sensor electrode as claimed in claim 4 characterised in that the glucose dehydrogenase is separated from Acinetobacter calcoaceticus.

6. A sensor electrode as claimed in any of claims 1 to 5 characterised in the mediator compound is a polyyviologen, o-chloranil, or a ferrocene-type compound.

7. A sensor electrode as claimed in claim 6 characterised in that the ferrocene-type compound is ferrocene itself 1,1'-ferrocenedicarboxylic acid, dimethyl ferrocene, or polyvinyl ferrocene.

8. A sensor electrode as claimed in any of claims 1 to 7 characterised in that the electrode is made of silver, of a carbon particle paste or of solid carbon.

9. A sensor electrode as claimed in any of claims 1 to 8 characterised by the particular combination in which the electrically conductive material is carbon, the mediator compound is a layer of ferrocene or a ferrocene derivative and the enzyme is a glucose oxidase or bacterial glucose dehydrogenase located upon the layer of mediator compound.

10. A sensor electrode as claimed in claim 9 characterised in that the ferrocene or ferrocene derivative is in monomeric or polymeric form and deposited from a readily evaporatable organic solvent therefor; or in polymeric form and produced at the surface by polymerisation of the corresponding monomer; or is bonded to the carbon electrode by carbo-diimide cross-linking.

11. A sensor electrode as claimed in claim 9 or 10 characterised in that the enzyme is a glucose oxidase immobilised on the mediator by DCC.

12. A sensor electrode as claimed in claim 9 or 10 characterised in that the enzyme is a bacterial glucose dehydrogenase either deposited on the mediator layer from an evaporatable solution, or held in a gelatine layer at the surface of the mediator layer.

13. A sensor electrode as claimed in any of claims 9 to 12 characterised by having an outermost protective membrane permeable to water and glucose molecules, such as a layer of cellulose acetate deposited from a solution thereof.

14. A sensor electrode as claimed in any one of the proceeding claims 1 to 13 in combination with temporary or permanent implantation means such as a needle-like probe.

15. A sensor electrode combination as claimed in claim 14 in further combination with signal or control equipment.

1/2

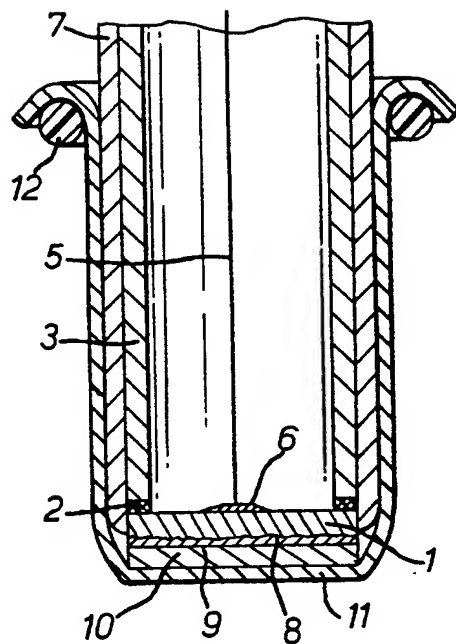


FIG. 1.




FIG. 2.

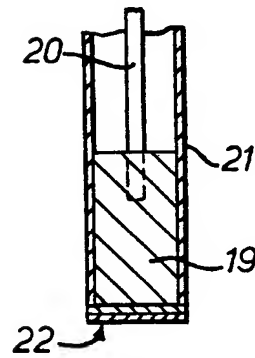


FIG. 5.

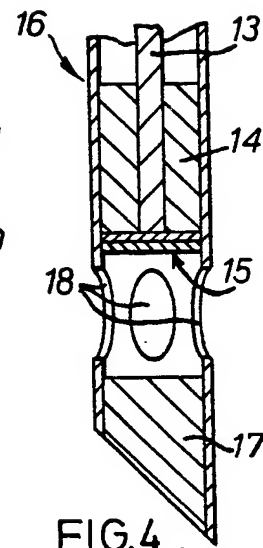


FIG. 4.

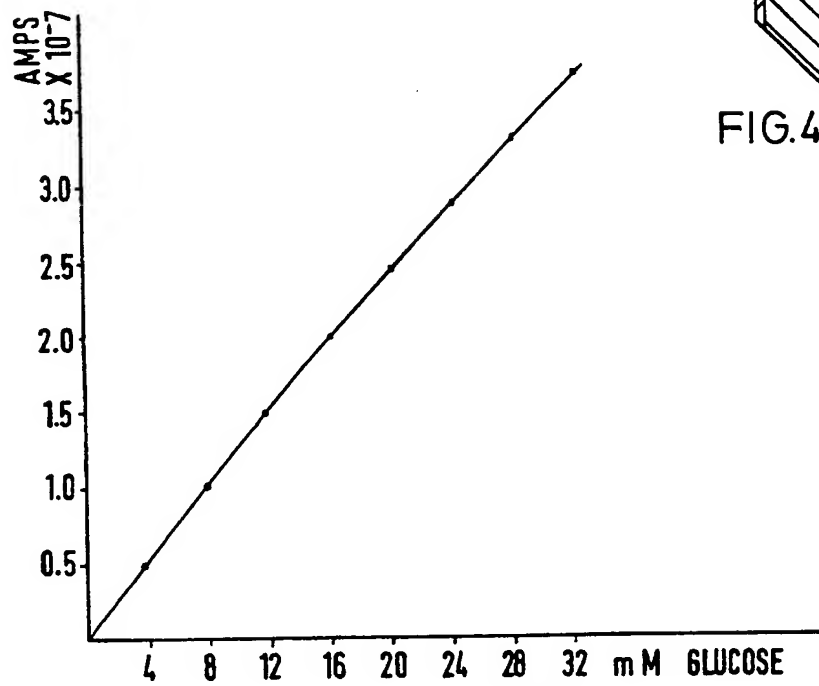


FIG. 3.

2/2

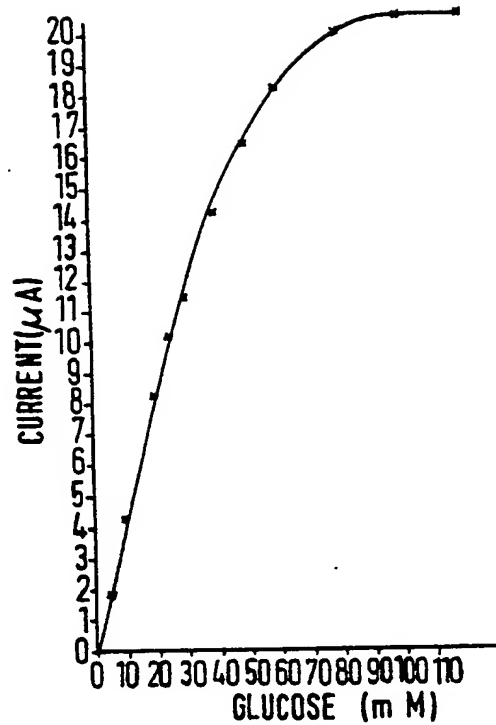


FIG.6.

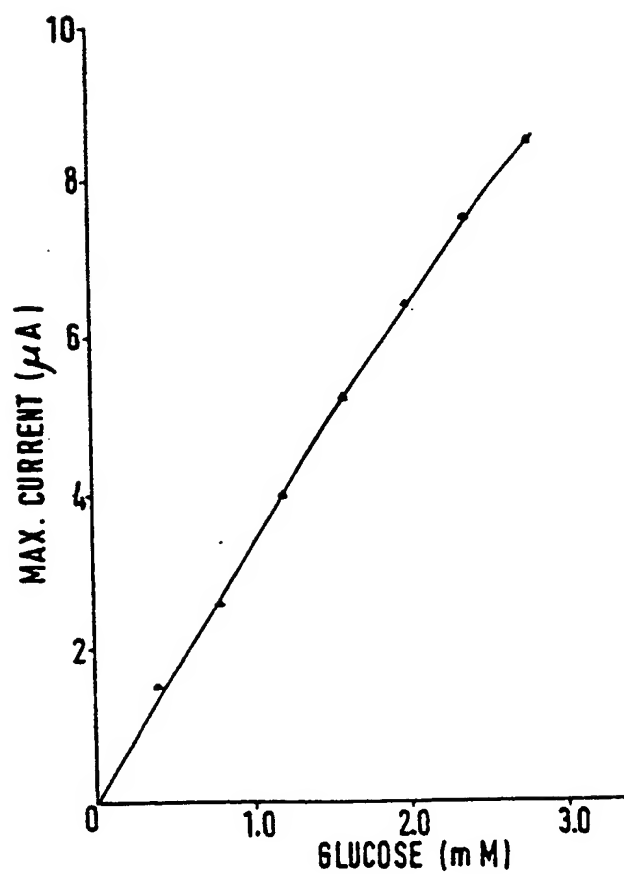


FIG.7.



European Patent  
Office

# EUROPEAN SEARCH REPORT

0078636

Application number

EP 82 30 5597

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int. Cl. 3)
Y	<p>--- US-A-4 144 143 (F.M. HAWKRIDGE et al.) * Columns 1, 2 ; column 3, lines 1-34 *</p>	1-4, 6, 7, 12	G 01 N 27/30 G 01 N 33/48
Y, P	<p>--- DD-A- 154 041 (ADW DER DDR) * Claim 1 ; page 2 *</p>	1-4, 12	
Y	<p>--- ANALYTICAL CHEMISTRY, vol. 51, no. 1, January 1979 T. SHINBO et al. "Potentiometric enzyme electrode for lactate", pages 100-101 * Pages 100-101 -----</p>	6, 7	
			TECHNICAL FIELDS SEARCHED (Int. Cl. 3)
			G 01 N 27/00 G 01 N 33/00
The present search report has been drawn up for all claims			
Place of search BERLIN		Date of completion of the search 21-01-1983	Examiner DIETRICH A.
<p><b>CATEGORY OF CITED DOCUMENTS</b></p> <p>X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document</p> <p>T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application L : document cited for other reasons &amp; : member of the same patent family, corresponding document</p>			